

Display Report

Analysis Info


Analysis Name D:\data\engele\CS017651_BE1_01_7991.d
Method 1008-ms.m
Sample Name CS017651
Comment

Acquisition Date 7/22/2022 6:12:23 PM

Operator Demo User
Instrument impact II 1825265.10256

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	2600 V	Set Dry Heater	180 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	10000 m/z	Set Charging Voltage	2000 V	Set Divert Valve	Source
		Set Corona	0 nA	Set APCI Heater	0 °C

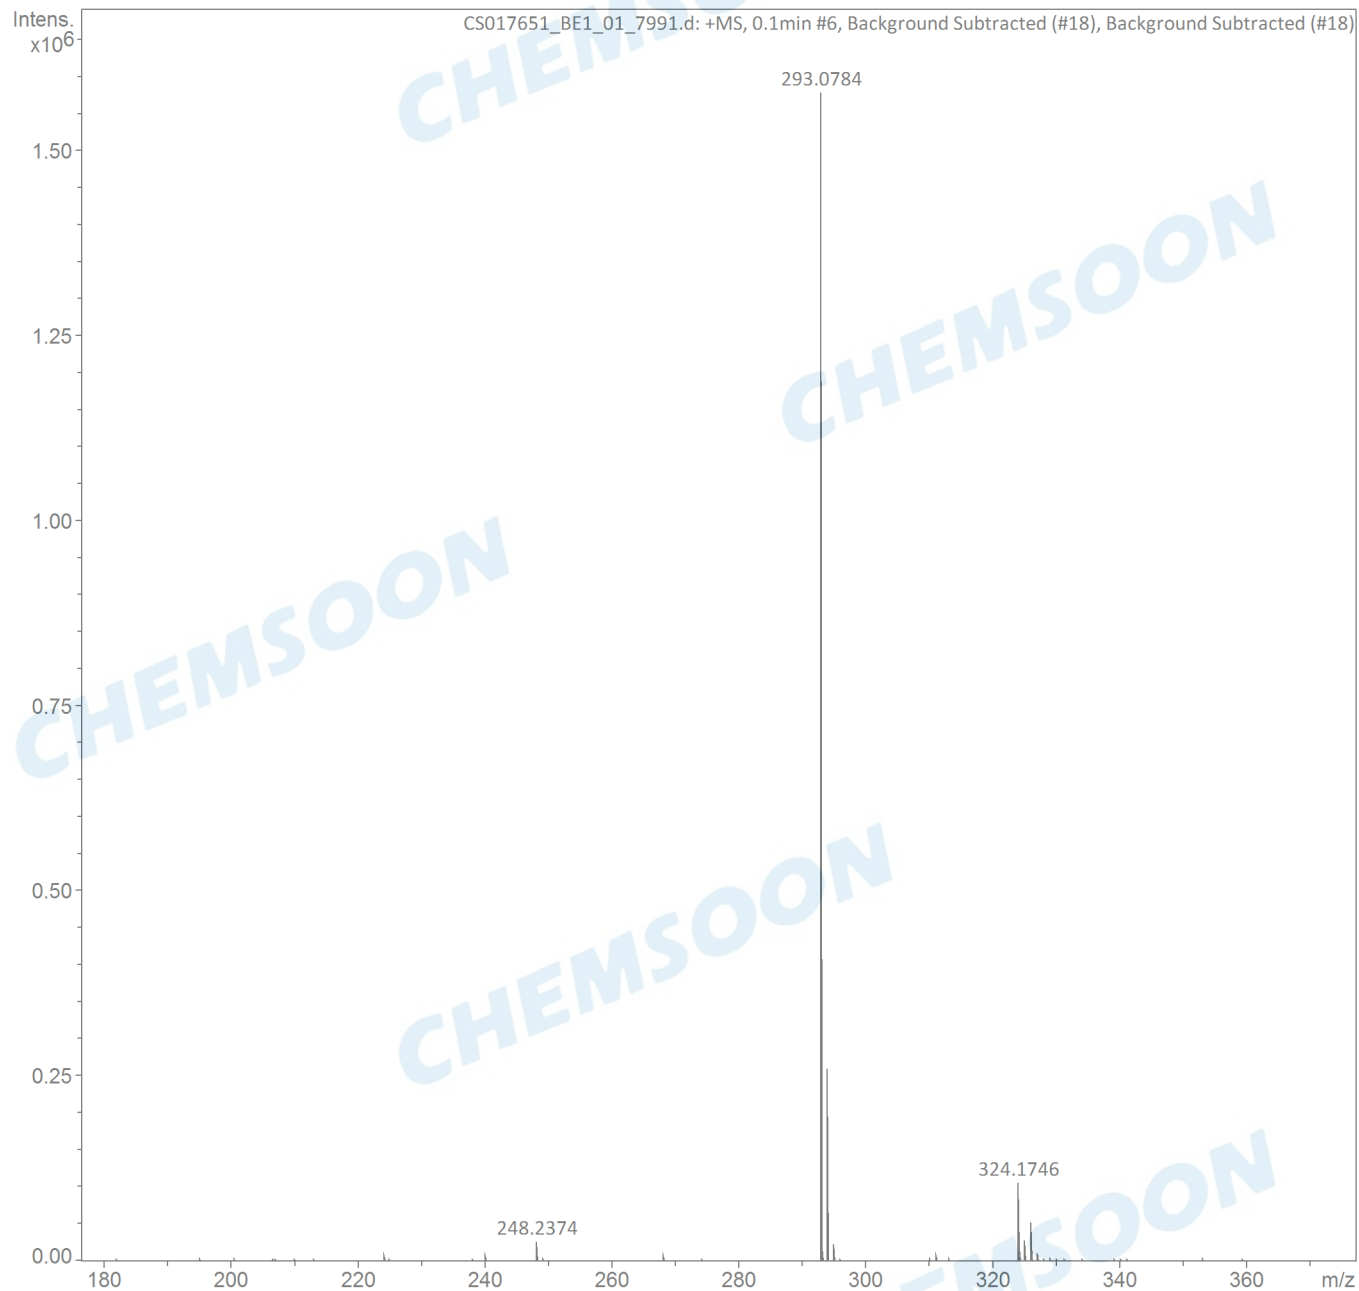

CS017651_BE1_01_7991.d

Bruker Compass DataAnalysis 4.4

printed: 7/22/2022 6:17:50 PM

by: demo

Page 1 of 1