

Display Report

Analysis Info


Analysis Name D:\Data\engle\CS017076_RA5_01_9604.d
Method 1225-1.m
Sample Name CS017076
Comment

Acquisition Date 9/2/2021 9:11:20 AM

Operator Demo User
Instrument impact II 1825265.10256

Acquisition Parameter

Source Type	ESI	Ion Polarity	Positive	Set Nebulizer	0.4 Bar
Focus	Not active	Set Capillary	2600 V	Set Dry Heater	180 °C
Scan Begin	50 m/z	Set End Plate Offset	-500 V	Set Dry Gas	4.0 l/min
Scan End	3000 m/z	Set Charging Voltage	2000 V	Set Divert Valve	Source
		Set Corona	0 nA	Set APCI Heater	0 °C

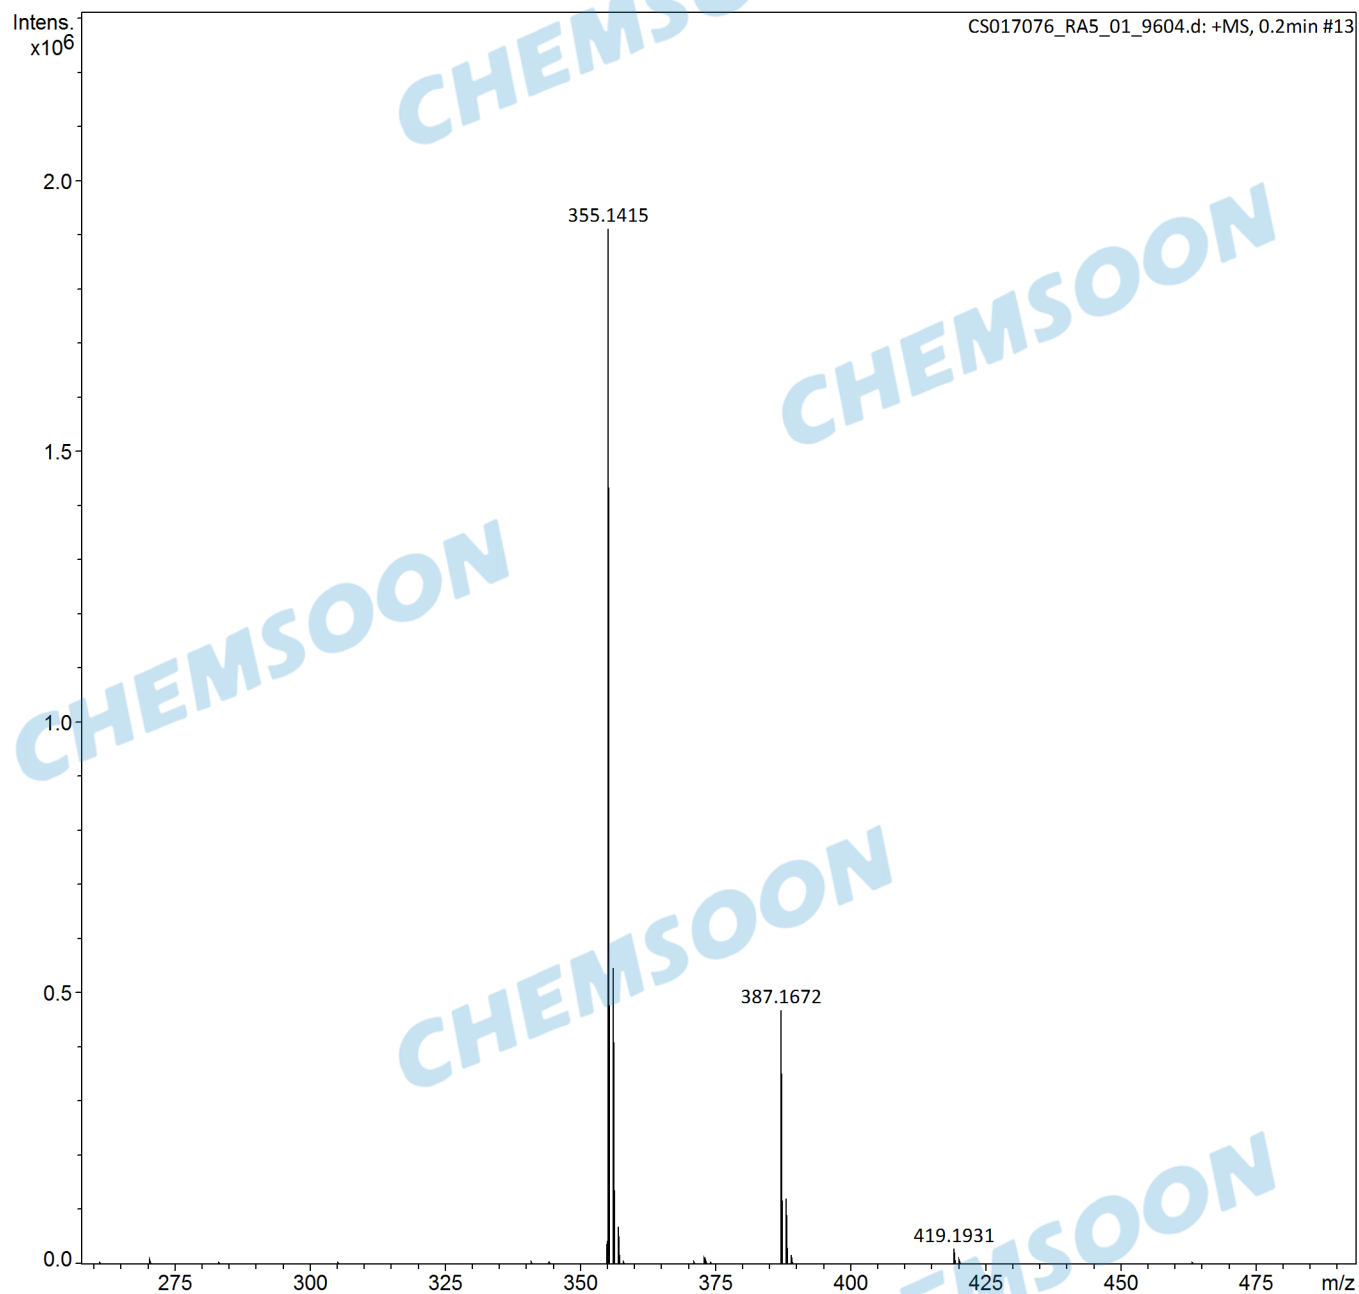

CS017076_RA5_01_9604.d

Bruker Compass DataAnalysis 4.4

printed: 9/2/2021 9:13:01 AM

by: demo

Page 1 of 1